


## EMResource® 4.4 Release Notes

These notes describe highlights of the EMResource 4.4 release scheduled for Wednesday, July 20, 2022. More information is available through the help in your solution or by contacting the Juvare Support at 877-771-0911 or [support@juvare.com](mailto:support@juvare.com).

### Status Reasons User Interface


Now, the Status Reasons page has an updated interface to help you more effectively create, edit, and organize status reasons. You can adjust the display of status reasons by hiding or showing columns and filtering column data, making it easier to find the information you need.

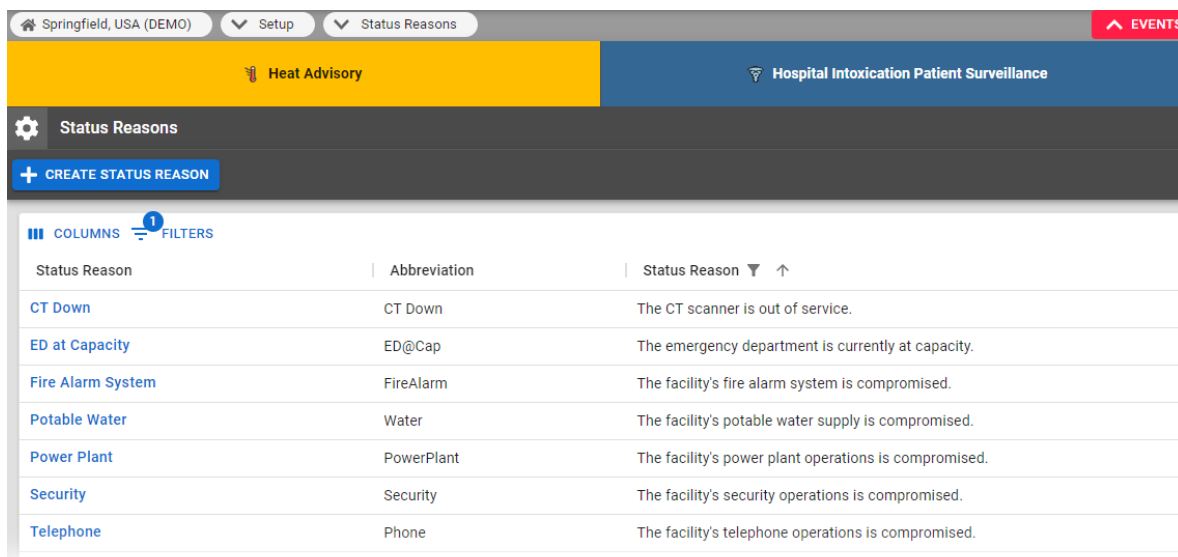

The screenshot shows the 'Status Reasons' page in a web application. At the top, there are navigation tabs for 'Springfield, USA (DEMO)', 'Setup', and 'Status Reasons'. Below this is a header with 'Heat Advisory' and 'Hospital Intoxication Patient Surveillance'. A 'Status Reasons' section contains a '+ CREATE STATUS REASON' button. Below that, there are 'COLUMNS' and 'FILTERS' options. The main content is a table with three columns: 'Status Reason', 'Abbreviation', and 'Status Reason'. The table lists several status reasons with their corresponding abbreviations and descriptions.

Status Reason	Abbreviation	Status Reason
CT Down	CT Down	The CT scanner is out of service.
ED at Capacity	ED@Cap	The emergency department is currently at capacity.
Fire Alarm System	FireAlarm	The facility's fire alarm system is compromised.
Potable Water	Water	The facility's potable water supply is compromised.
Power Plant	PowerPlant	The facility's power plant operations is compromised.
Security	Security	The facility's security operations is compromised.
Telephone	Phone	The facility's telephone operations is compromised.

Additionally, when viewing status reasons, you can edit a status reason and use the navigation buttons to continue to the next one without going back to the main Status Reasons page.

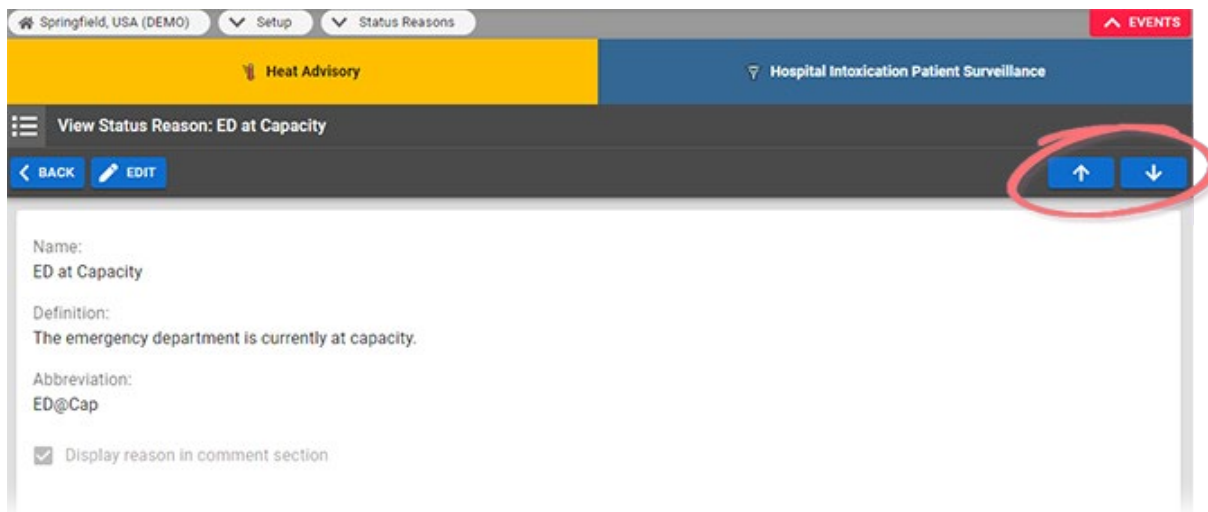

The screenshot shows the 'View Status Reason: ED at Capacity' page. At the top, there are navigation tabs for 'Springfield, USA (DEMO)', 'Setup', and 'Status Reasons'. Below this is a header with 'Heat Advisory' and 'Hospital Intoxication Patient Surveillance'. The main content area shows the details for the 'ED at Capacity' status reason, including its name, definition, and abbreviation. There are 'BACK' and 'EDIT' buttons. A red circle highlights two navigation buttons (up and down arrows) located at the bottom right of the page.

Name:  
ED at Capacity

Definition:  
The emergency department is currently at capacity.

Abbreviation:  
ED@Cap

Display reason in comment section

## Resolutions

- On iOS mobile devices, an issue that prevented the sound associated with a notification was resolved.
- An issue that occurred when importing large files through Bulk Upload was resolved.